



Journal Homepage: [-www.journalijar.com](http://www.journalijar.com)

INTERNATIONAL JOURNAL OF ADVANCED RESEARCH (IJAR)

Article DOI: 10.21474/IJAR01/18791

DOI URL: <http://dx.doi.org/10.21474/IJAR01/18791>



RESEARCH ARTICLE

REPEAT RADIOGRAPHY ANALYSIS AND CORRECTIVE MEASURES IN A PRIVATE MEDICAL COLLEGE AND TEACHING HOSPITAL

Mahima Dwivedi¹, Mayuri Ojah^{2*}, Meghna Guha³

1. Assistant Professor, Department of Medical Imaging, Quantum University
2. Assistant Professor, Department of Radiography and Advance Imaging Technology, the Assam Royal Global University, Betkuchi, Guwahati-35, Assam, India.
3. Assistant Professor, Radiography and Advance Imaging Technology, the Assam Royal Global University, Betkuchi, Guwahati-35, Assam, India.

Manuscript Info

Manuscript History

Received: 25 March 2024

Final Accepted: 30 April 2024

Published: May 2024

Abstract

Aims and objectives: The primary goal of this study is to identify the body parts that undergo repeated radiographic examinations the most frequently and the prevalent causes of these examinations.

Materials and Methods: A prospective study was carried out in the Department of Radio-Diagnosis and Imaging to investigate the reasons behind repeated radiography in a private university hospital in India. A total of 6832 samples were evaluated between November 1, 2021, and April 30, 2022.

Discussion: Repetition of a patient's radiographic projection can be caused by several circumstances.

The common factors found in this study are collimation error, wrong centering, patient motion and incorrect positioning, appearance of artifacts owing to insufficient patient preparation at times and patient non-cooperation like patient motion. Repeat radiographs using the computed radiography technology are influenced by a plethora of circumstances. These variables include technical parameters chosen, the patient's Body Mass Index (BMI) and the patient's level of preparation.

Conclusion: Repeat radiography plays an important role as a key indicator in evaluating the quality of the service provided by the medical imaging department and gives us an insight on whether the dose rates are within the given guidelines or not.

Copy Right, IJAR, 2024,. All rights reserved.

Introduction:-

Studies done on animals and by early radiologists has so far established that ionizing radiation is a carcinogen. "Ionizing radiation refers to nuclear radiation consisting of subatomic particles or electromagnetic waves with sufficient energy to ionize atoms or molecules by stripping them of electrons. This category includes gamma rays, X-rays, and the more energetic ultraviolet part of the electromagnetic spectrum." [1]. The discovery of x-ray, radium and radioactivity during the late 19th century has led to remarkable developments in the clinical, technological and experimental experiments in the medical imaging sector and has continued to benefit the field of medicine. However, a few years after the first x-ray exposures were made for imaging the human body, physicians, scientists and medical radiation workers started developing several adverse health conditions like dermatitis, cataracts, skin

Corresponding Author:- Ms. Mayuri Ojah

Address:- Department of Radiography & Advance Imaging Technology, the Assam Royal Global University, Betkuchi, Opp. Guwahati-35, Assam, India.

carcinomas, leukemia and others. Little was known during those early occurrences that those effects could have been due to the ionizing radiation with which they were working. It took around twenty five years to form radiation protection committees and to implement the first recommendations that were made to decrease the stray radiation and minimize the x-ray beam to the patient[8]. The US population's exposure to medical radiation has increased by 600% since 1980, and there may be future cancer risks for these patients, despite the enormous benefits [10]. With the advent of radiation protective devices, dose rate monitoring and measuring equipment, the occupational dose rates have significantly lessened. However epidemiological studies done between 1956 to the present time have linked diagnostic x-rays with the increased number of cancer cases in patients [2] which includes occurrence of pediatric leukemia in offspring of mothers undergoing diagnostic x-rays during pregnancy and increased breast cancer risks in women with tuberculosis monitored using Fluoroscopy [3-6] and in women with scoliosis evaluated with repeated x-rays. [7]

Radiographs are repeated to obtain the diagnostic information required to diagnose, which is the primary motive of irradiating a patient. Radiation doses resulting from X-ray examinations depend on the X-ray imaging technology and the exposure setting employed for recording the images on these imaging devices [3,4]. However, X-ray imaging is the largest contributor to population dose because a large number of X-ray examinations are conducted every year globally[5]. Diagnostic procedures accounts for more than 95% of medical exposure to radiation worldwide [6]. The main objective of an x-ray examination is to project radiographic features of anatomic detail of an examined body part with optimal exposure factors with the lowest possible radiation dose to the patient. Although at times, owing to many different factors such as technical errors, wrong exposure factors, non-complying patients, etc, radiographs need to be repeated. This leads to the patients receiving an additional amount of radiation dose. Although justification is attained here but overall the principle of ALARA (as low as reasonably achievable) is not achieved. In addition to the imaging techniques exposing patients to ionizing radiation, probable danger of allergic reactions or complications from intravenous contrast agent use are also there [9]. Repeat radiographs are a sign of dearth of skilled professionals and reflect defectively on the technologists as well as the department. Retaking radiological exam images not only puts patients at greater danger of radiation exposure, but it also wastes medical resources and lowers hospital service quality [11]. Repeat analysis of radiographs is a subjective evaluation of the quality of x-ray image where the films considered to be of poor quality are categorized according to their cause. This study aims to find the rate of repeated radiographs for digital radiography, the most commonly repeated types of body parts and the causes of repetition for fixed radiography.

Materials and Methods:-

Ethics:

The Standing Committee for Scientific Research at the medical college granted an exemption from a comprehensive ethical assessment because all the data were gathered retrospectively and anonymized. For this investigation, written informed consent was obtained from each and every technician involved.

Design/Setting:

A retrospective longitudinal study of data was collected from November 2021 to April 2022. The data were collected (n = 6,832 x-ray images) for a period of six months.

Procedure:

The data collection was achieved with the help of radiographers and medical imaging students of the radiology department. The data collectors were provided with basic training and have been briefed about the objectives of the study and in what way it will benefit the society at large. The repeated studies were discerned from the imaging software, which were then evaluated. The cause of rejecting those films and the errors made were compared to the repeated and accepted x-ray films to establish the reasons of repeat.

Data analysis:

Secondary analysis of the raw data was conducted using Microsoft Excel 2010. The average repetition rate was calculated by the total number of repeat exposure multiplied by 100 and the product is divided by the total number of procedures performed. This formulae was recommended as per NABH 5th edition.

Table 1:-

Repeat rate for each examination type			
Examination type	Repeated	Total images acquired	Repeat rate (%)
CHEST AP	116	2865	4%
C-SPINE	24	286	8%
DL SPINE	7	220	3%
LS SPINE	57	480	12%
FINGER	2	68	3%
HAND	12	130	9%
WRIST	9	150	6%
FOREARM	4	99	4%
ELBOW	1	16	6%
ARM	0	20	0%
SHOULDER	19	27	70%
HIP	3	30	10%
THIGH	5	100	5%
KNEE	3	156	2%
LEG	2	56	4%
ANKLE	2	236	1%
FOOT	12	136	9%
ABDOMEN	17	700	2%
PELVIS/KUB	12	650	2%
Mastoid	1	235	0%
PNS	1	54	2%
KUB	3	118	3%

C: Cervical, DL: Dorso-lumbar, LS: Lumbo-Sacral, PNS: Paranasal sinus, KUB: Kidney Ureter Bladder

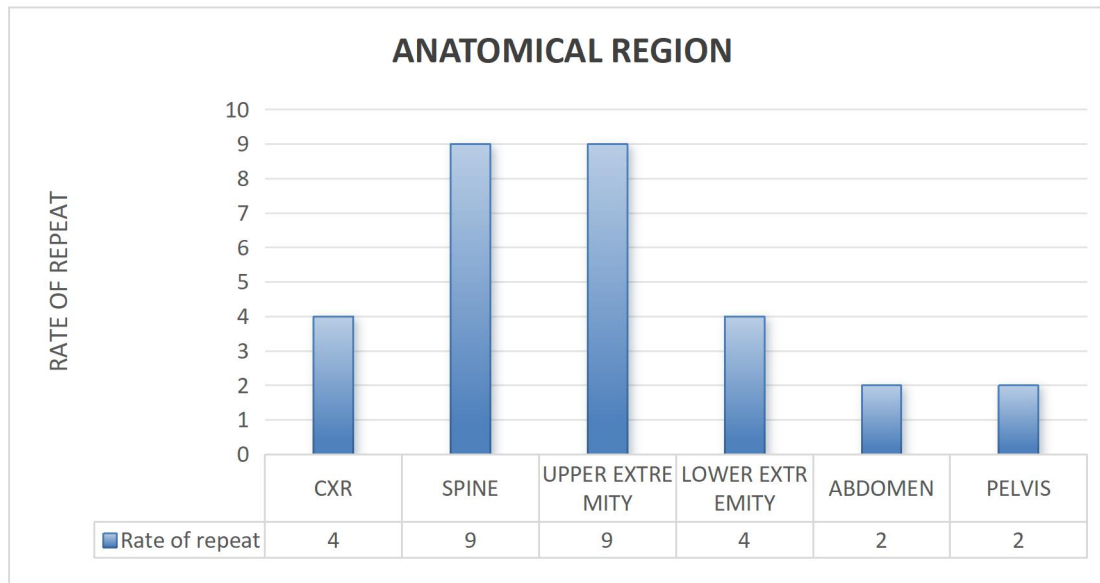


Figure 1:- Total number of repeated exposures according to body part.

Result:-

Table 1 and Figure 1 shows the total number of repeated exposures and their repeat rates according to different anatomical regions. Figure 2 gives us an overview of the most frequently identified reasons of image repetition with the most common reason owing to collimation error, followed by wrong centering, patient motion and incorrect positioning. The other reason of repetition includes artifacts, anatomy cut-off, absence of marker and patient not holding breath during exposure.

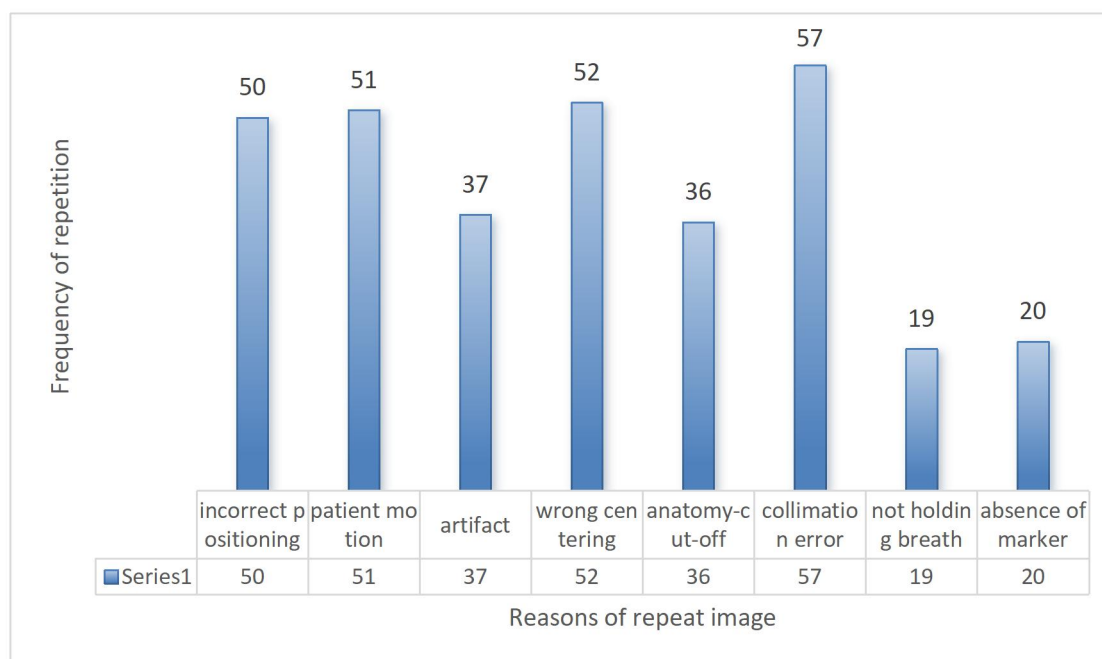


Figure 2:- The identified reasons for repeat images and the number of repetition.

The overall repetition rate was 7.55% which includes all the investigations gathered during this study. For chest x-ray (both PA and AP views), a total of 116 out of 2865 were found to be repeated. In case of upper and lower extremities, the repetition rates were 9% and 4% respectively. The repetition rate in case of spine was found to be 9% as well and 2% rate was found for both abdomen and pelvis. Out of the commonly identified reasons of repeat, the most common cause was collimation error and wrong centering, followed by patient motion and incorrect positioning. Other identified reasons were artifact, anatomy cut-off, absence of marker and patient not holding breath properly during exposure.

Discussion:-

The purpose of this study was to look into the rates of diagnostic medical image repetition and to identify areas that needed improvement in the medical imaging departments. There are a number of reasons which contributed to the 7.55% of repetition. After evaluation, it was found that some of the anatomical parts had repeat rate as high as 70% (shoulder) and some as low as 1% (ankle). Also it was found that for arm, there was no repetition. This only suggests that some anatomical parts are more commonly repeated than others owing to many factors which may include complex patient position, tube angulation, technician skill level etc. In a similar study, the overall reject rate was found to be 8.96%, with hip recording the highest percentage of reject (20%), followed by elbow (15.2%) [13]. Yet in another study, the repeat rate was only found to be 1.87% with Pelvis recording the highest percentage of repeat (12.50%), followed by chest (1.40%) [14]. It has been noticed that the reject rates were greater than the average procedure for several anatomical areas and found to vary in different research studies. The variation in the number of repeat rates could be attributed to a multitude of factors such as technologist's level of expertise, their clinical experience, how well the machines were calibrated, quality control and assessment, etc. Thus, prioritizing internal training on equipment maintenance, quality control, workshops and training programs in these specific anatomical areas which need to be optimized by assessing the rejection rates is crucial for each examination and projection, and find out ways to make the projection easier to expose thereby improving the quality of radiographs and reducing the overall exposure to the patients as well as staff.

Conclusion:-

The objectives of the study have been met, and during the course of its 5-month duration, an average reject rate of 7.55% was discovered. The department's performance could not be accurately represented by a single percentage, and a deeper analysis of individual projections and radiographer reject rates need to be determined and an effective way to lower reject rates and patient dose is to be established. Reject analysis changes the workflow, lowers patient dose, increases departmental efficiency and helps in directing the staff education and training [12]. The authors

recommend that for internal education programs, the medical imaging department may implement more uniform image quality standards and a feedback system. To monitor and lower patient exposure to ionizing radiation, exposure index data collection would be beneficial for future investigations into reject analysis. It should also be kept in mind to incorporate the radiation principles like ALARA (As Low As Reasonably Achievable) and TDS (Time Distant Shielding) while working with patients in the medical imaging department.

Funding:

None.

Conflicts of Interest:

No conflict of interest has been declared by any author.

Reference:-

1. Kelly BS, Judge C, Bollard SM, Clifford SM, Healy GM, Aziz A, Mathur P, Islam S, Yeom KW, Lawlor A, Killeen RP. Radiology artificial intelligence: a systematic review and evaluation of methods (RAISE). *Eur Radiol.* 2022 Nov;32(11):7998-8007. doi: 10.1007/s00330-022-08784-6. Epub 2022 Apr 14. Erratum in: *Eur Radiol.* 2022 May 20; PMID: 35420305; PMCID: PMC9668941.
2. Ron, Elaine. CANCER RISKS FROM MEDICAL RADIATION. *Health Physics* 85(1):p 47-59, July 2003.
3. Boice JD Jr, Preston D, Davis FG, Monson RR. Frequent chest X-ray fluoroscopy and breast cancer incidence among tuberculosis patients in Massachusetts. *Radiat Res.* 1991; 125:214-222. [PubMed: 1996380]
4. Howe GR, McLaughlin J. Breast cancer mortality between 1950 and 1987 after exposure to fractionated moderate-dose-rate ionizing radiation in the Canadian fluoroscopy cohort study and a comparison with breast cancer mortality in the atomic bomb survivors study. *Radiat Res.* 1996; 145:694-707. [PubMed: 8643829]
5. Ron E. Cancer risks from medical radiation. *Health Phys.* 2003; 85:47-59. [PubMed: 12852471]
6. Boice, JD, Jr.. Ionizing radiation. In: Schottenfeld, D.; Fraumeni, JF., Jr., editors. *Cancer Epidemiology and Prevention*. 3rd ed. Oxford University Press; New York: 2006. p. 259-293.
7. Doody MM, Lonstein JE, Stovall M, Hacker DG, Luckyanov N, Land CE. Breast cancer mortality after diagnostic radiography: findings from the U.S. Scoliosis Cohort Study. *Spine. (Phila Pa 1976)*. 2000; 25:2052-2063. [PubMed: 10954636]
8. Hendee WR, O'Connor MK. Radiation risks of medical imaging: separating fact from fantasy. *Radiology.* 2012 Aug;264(2):312-21. doi: 10.1148/radiol.12112678. PMID: 22821690.
9. Scatliff JH, Morris PJ. From Roentgen to magnetic resonance imaging: the history of medical imaging. *N C Med J.* 2014 Mar-Apr;75(2):111-3. doi: 10.18043/ncm.75.2.111. PMID: 24663131.
10. Linet MS, Slovis TL, Miller DL, Kleinerman R, Lee C, Rajaraman P, Berrington de Gonzalez A. Cancer risks associated with external radiation from diagnostic imaging procedures. *CA Cancer J Clin.* 2012 Mar-Apr;62(2):75-100. doi: 10.3322/caac.21132. Epub 2012 Feb 3. Erratum in: *CA Cancer J Clin.* 2012 Jul-Aug;62(4):277. PMID: 22307864; PMCID: PMC3548988.
11. Guidelines for reducing image retakes of general digital radiography Chih-Sheng Lin, Po-Chou Chan, Kuang-Hua Huang, Chun-Feng Lu, Yung-Fu Chen and Yun-O Lin Chen
12. Stephenson-Smith B, Neep MJ, Rowntree P. Digital radiography reject analysis of examinations with multiple rejects: an Australian emergency imaging department clinical audit. *J Med Radiat Sci.* 2021 Sep;68(3):245-252. doi: 10.1002/jmrs.468. Epub 2021 Apr 7. PMID: 33826800; PMCID: PMC8424327.